


STANDARD F

Dengue IgM/IgG FIA SD BIOSENSOR

STANDARD F Dengue IgM/IgG FIA qualitatively analyzes Dengue virus specific IgM and IgG antibodies in serum, plasma and whole blood using fluorescent immunoassay. Screening test results can be obtained within 15 minutes with high sensitivity and specificity.

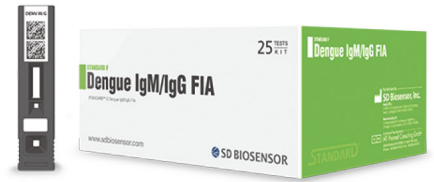


CE


Specification

Intended use	Qualitative detection of Dengue virus-specific IgM and IgG antibodies
Specimen Type	Whole blood, Serum, Plasma
Specimen Volume	10 μ l
Testing Time	15 mins.
Storage Conditions	2-30°C / 36-86°F

STANDARD TEST MODE

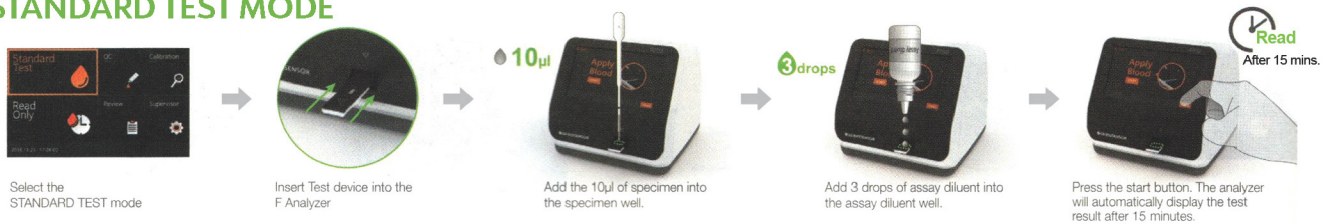

READ ONLY MODE

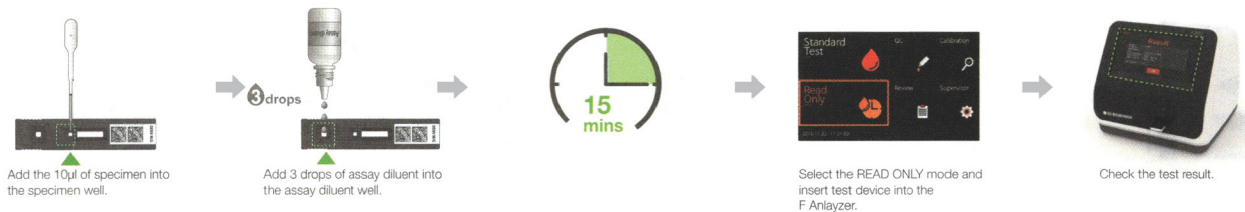

TEST PERFORMANCE

Reference	Sensitivity	Specificity
ELISA	98% (42/43)	99% (183/184)

ORDERING INFORMATION

Category	Sensitivity	Pack Size
Vector Borne	Standard F Dengue IgM/IgG FIA	25 Test